

Monitor adaption

Colours to choose CD

Max. load capacity support arm Max. load monitor adaptation Product weight

Part number

prepared to accept Philips table top mount

decorative parts RAL 5013 cobalt blue / RAL 7024 graphite grey aluminum parts RAL 9016 traffic white / RAL 9002 grey white

18 kg / 39.7 lbs 18 kg / 39.7 lbs 3.0 kg/ 6.6 lbs

A-H33030PH-Y.CD

Fixings Y



Adapter for vertical wall channel



Adapter for Mindray medical supply units

2F

Horizontal rail clamp



Adapter for Amico pendants & headwalls

details page 3



Vertical rail clamp



Adapter for Dräger Ambia pendants & headwalls



Universal pole clamp



1B 1F

Fixed pole clamp



Adapter for Löwenstein Medical / ITD / mounting channel

CIM-MED.COM






Extended pivot arm heavy duty

Technical data

SIDE VIEW

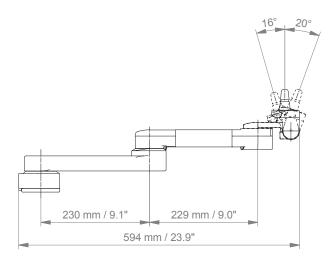

TOP VIEW

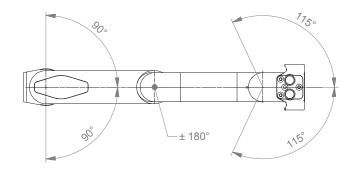








Illustration	Description	Notes	Weight	Part no.
	Adapter for vertical wall channel	To mount to CIM wall channel (compatible with GCX channel) Please order separately: CIM wall channel, see catalogue accessoires	0.6 kg / 1.3 lbs	4 S
	Horizontal rail clamp	To mount to horizontal European rails 10 x 25, 8 x 35, 10 x 30, 10 x 50 mm	1.1 kg / 2.4 lbs	2F
	Vertical rail clamp	To mount to vertical European rail 10 x 25 mm	0.5 kg / 1.1 lbs	3
	Universal pole clamp	V-block to mount to pole ø 23 - 40 mm / 0.9 - 1.6"	0.6 kg / 1.3 lbs	1V
	Fixed pole clamp	To mount to pole ø 25 mm / 1.0" To mount to pole ø 30 mm / 1.2" To mount to pole ø 35 mm / 1.4" To mount to pole ø 38 mm / 1.5"	0.3 kg / 0.7 lbs 0.4 kg / 0.9 lbs 0.4 kg / 0.9 lbs 0.4 kg / 0.9 lbs	1 1B 1F 1C
	Adapter medical supply units	For Mindray medical supply units	0.8 kg / 1.8 lbs	13
+ 111	Adapter pendants & headwalls	For Amico pendants & headwalls	0.6 kg / 1.3 lbs	17
::0	Adapter pendants & headwalls	For Dräger Ambia pendants & headwalls	0.6 kg / 1.3 lbs	19
1	Adapter pendants & headwalls	For Löwenstein Medical / ITD / mounting channels	0.4 kg / 0.9 lbs	9



How to create part numbers

Part numbers can be easily created by following the steps below:

Please replace the letters in green with the part no. code as per your requirements.

1. Components' grounding:

 $\mathsf{A} \qquad \qquad \mathsf{=} \qquad \mathsf{grounded}$

2. Choose the arm version required:

224PH / 230PH = pivot arm

33030PH = extended pivot arm light duty H33030PH = extended pivot arm heavy duty

431PH = height adjustable arm

73130PH = extended height adjustable arm 531PH = high position height adjustable arm

83130PH = extended high position height adjustable arm

224FMS / 230FMS = pivot arm, FMS interface

32424FMS / 33030FMS = extended pivot arm light duty, FMS interface

224MP2 / 230MP2 = pivot arm, MP2/ X2/ X3 interface

224MP2PS / 230MP2PS = pivot arm, MP2/ X2/ X3 interface with power supply enclosure

33030MP2 = extended pivot arm light duty, MP2/ X2/ X3 interface

33030MP2PS = extended pivot arm light duty, MP2/ X2/ X3 interface with power supply

224X2X3 / 230X2X3 = pivot arm, without cable hook, MP2/ X2/ X3 interface

= extended pivot arm light duty, without cable hook, MP2/ X2/ X3 interface

431X2X3 = height adjustable arm, without cable hook, MP2/ X2/ X3 interface with power supply enclosure

73130X2X3 = extended height adjustable arm, without cable hook, MP2/ X2/ X3 interface

3. Specify where you want to mount the arm and select the fixing (Y):

1V = pole \emptyset 23 - 40 mm / 0.9 - 1.6" 1 = pole \emptyset 25 mm / 1.0" 1B = pole \emptyset 30 mm / 1.2"

1F = pole ø 35 mm / 1.4" 1C = pole ø 38 mm / 1.5"

2F = horizontal rails 10 x 25, 8 x 35, 10 x 30, 10 x 50 mm

3 = vertical rail 10 x 25 mm 4S = vertical wall channel

9 = Löwenstein Medical / ITD / mounting channel

13 = Mindray medical supply units 17 = Amico pendants & headwalls

19 = Dräger Ambia pendants & headwalls



How to create part numbers

4. Choose the colour requested for decorative parts (C):

gr = RAL 7024 (graphite grey) graphite = RAL 5013 (cobalt blue)

5. Choose the colour requested for the aluminium die-cast parts (D):

1 = RAL 9016 (traffic white) 2 = RAL 9002 (grey white)

6. Specify the spring depending on the weight of your monitor/ device - only with height adjustable arms (X):

0 - 3.5 kg / 0 - 7.7 lbs (only for MP2/ X2/ X3)60 2 - 5 kg / 4.4 - 11 lbs= 95 4 - 9 kg / 8.8 - 19.8 lbs 110 4.5 - 12.5 kg / 9.9 - 27.6 lbs 130 7.5 - 13 kg / 16.5 - 28.7 lbs = 160 12.5 - 19 kg / 27.6 - 41.9 lbs 175 13 - 16 kg / 28.7 - 35.3 lbs 220 16 - 22 kg / 35.3 - 48.5 lbs =

Example

01 Grounding		02 Arm version		03 Fixing	04 & 05 Colour		06 Spring tension
A	_	431PH	_	Υ	CD	_	X
A	-	431PH	_	4S	gr1	_	95

CIM-MED.COM





Monitor adaptations

All mounting systems for **Philips IntelliVue series** are prepared to accept the Philips table top mount.

Mounting solutions for the **Efficia series** and **Sure Signs**/ **Vital Signs** are shown in the catalogue "5" plunge plate adaptation".

Please note!

The Philips table top mount must be ordered separately by Philips.

Components' grounding

All arms with integrated cable management are equipped with **component grounding**. No grounding is required for arms with external or semi-integrated cable management with cables not being led through joints.

Load capacity

All height adjustable arms have a load capacity of 22 kg / 48.5 lbs. Rear mounted monitor adaptations and horizontally mounted 5" plunge plates accept a maximum monitor weight of 18 kg / 39.7 lbs. An additional 4 kg / 8.8 lbs may be mounted on a down post underneath the front swivel part. Depending on material and tensile factor all weight indications have a 4-fold and/ or 6-fold safety factor according to IEC 60601-1 standards.

Custom-designed solutions and MRI applications

Please contact us for custom-designed solutions.

Product marking

All products which are classified as medical product risk class 1 are CE marked. As medical product risk class 1 they are conform with the regulations (EU) 2017/745 (MDR) and IEC 60601-1. Other standards of the IEC 60601 series are not applicable to our products, regardless of their version.

MD A stand-alone product that is already classified as a medical product class 1 before being integrated into an overall medical device. The product is CE-marked. A declaration of conformity is available.


Accessories or spare parts that have no independent function and are therefore not subject to the MDR. These products are not CE-marked. A declaration of conformity is not required.

Warranty

All CIM products have a 5-year warranty to be free of defects in material and fuctionality from the date of delivery.

How to find the right product for your needs?

No problem with our configurator https://cim-configurator.com

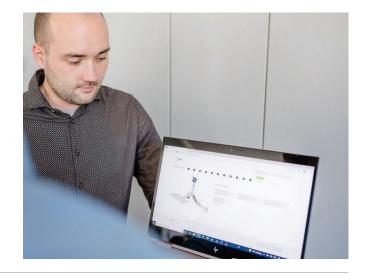



Product highlights

Non-height adjustable arm

Pivot and extended pivot arms offer full cable integration and easy cleaning for infection control in all critical care areas in the clinical environment. Our 5-years warranty guarantees reliable, trouble-free and maintenance-free operation. The swivel function at the fixing point as well as the tilt/swivel function of the monitor adaptation offers optimum positioning of your device. The extended pivot arm is a two-part arm with central pivot point between the two arm sections. All bottommounted monitors have the safety feature of a 20° tilt stop.

Height adjustable arm

The height adjustable arm offers **full cable integration**, one-wipe clean surfaces and our **5-year warranty** on the entirety of the product. Vertically and horizontally adjustable, the arm offers optimal positioning of your device. A constant viewing angle when vertically adjusted is guaranteed by a parallel linkage. **Weight-optimized springs counter-balance** the monitor without making any adjustments. All bottom-mounted monitors have the safety feature of a **20° tilt stop**. Individual rotational stops may be integrated in any joint.

To provide the perfect combination of arm and monitor, the CIM articulated height adjustable arm has a simple quarter-turn lock to hold the arm safely in position when removing the monitor. Furthermore the arm is equipped with the unique safety feature of a slow-release gas spring. Should anybody try to remove the monitor before locking the arm in position, the arm will only rise at a slow and even tempo.

